

## TEST OF SCINTILLATION COUNTERS FOR MULTICHANNEL TIME-OF-FLIGHT SYSTEM

S.V.Afanasiev, Yu.S.Anisimov, A.I.Malakhov,  
G.L.Melkumov, S.G.Reznikov, A.Yu.Semenov, P.I.Zarubin

The average time resolution ( $\sigma$ ) of about 70 ps is obtained for each of four scintillation counters at a long duration test on the CERN SPS particle beam. The counters were assembled of  $2.4 \times 2.4 \times 6.0$  cm<sup>3</sup> scintillator bars and FEU-87 (CsSb) type photomultipliers, both made in Russia. We observed the nonstability of mean time-of-flight (TOF) value during the runs. The maximum TOF drift contribution into the time resolution is estimated as (10—15)%.

The investigation has been performed at the Laboratory of High Energies, JINR.

Испытания сцинтилляционных счетчиков,  
предназначенных для создания  
многоканальных времяпролетных систем

С.В.Афанасьев и др.

В процессе долговременных испытаний набора из четырех сцинтилляционных счетчиков на пучке ускорителя SPS в ЦЕРНе получено среднее временное разрешение ( $\sigma$ ) порядка 70 пс для отдельного счетчика. Счетчики состояли из сцинтилляторов размерами  $2,4 \times 2,4 \times 6,0$  см<sup>3</sup> и фотомножителей типа ФЭУ-87 (CsSb), произведенных в России. Мы наблюдали нестабильность среднего значения времени пролета (TOF) на протяжении измерений. Максимальный вклад дрейфа TOF во временное разрешение оценен на уровне 10—15%.

Работа выполнена в Лаборатории высоких энергий ОИЯИ.

### 1. Introduction

This work was motivated by the planning of the NA49 experiment at CERN to research the new phenomena of Pb-Pb collisions at 200 GeV/amu [1]. Upon this Proposal the time-of-flight (TOF) counter system with about 70 ps time resolution is required to improve a separation of the pions, kaons and protons in momentum range 4-7 GeV/c to strengthen additionally the identification power provided by the time projection chambers.

The purpose of the test is to study the timing resolution of scintillation counters as a prototype for 1000-channel TOF detector wall on the negative particle wing. This is a continuation of our previous work [2,3], but the present TOF counters are manufactured of the batch of scintillators and photomultipliers procured for a mass production of the detectors.

## 2. Counter Design

We tested four TOF counters consisting of the plastic scintillator and the FEU-87 (CsSb) photomultiplier (PMT), both made in Russia. The scintillator was polystyrene doped with 3.5% PBD (phenyl-biphenyl-oxadiazol). Details of properties of this scintillation material are given in ref. [4]. Dimensions of the scintillation block were 6 cm (length)  $\times$  2.4 cm (width)  $\times$  2.4 cm (thickness in beam direction). In order to obtain the best value of the time resolution, we did not use the light guide. The PMT was coupled directly to the scintillator bar with an optical grease. The scintillator was wrapped in a black paper. The PMT has a 2 cm diameter CsSb photocathode and 11-stage dynode chain. We used special non-linear voltage divider [2] in this experiment. A voltage between the anode and the cathode of 2200 V provides electron gain of about  $10^7$  and output anode pulse of about 2V amplitude and 4 ns rise time for minimum ionizing particle.

## 3. Experimental Setup

The counters were tested in the H2 beam line of the CERN SPS north area with the following beams: protons of 200 and 30 GeV/c momenta and electrons of 20 GeV/c momentum. A schematic diagram of the measurements is shown in Fig.1. The counters under the test are  $S_1$ ,  $S_2$ ,  $S_3$  and  $S_4$ . Triggering was performed by three-fold fast coincidence of the start counter  $S_{\text{Start}}$  (quartz plate with Valvo XP2020 photomultiplier) and  $M_1$  and  $M_2$  counter signals. All electronics were placed in the NA49 counting room, and signals from the counters passed through 33 m long Suhner SO3272 coaxial cables and then were splitted into two equal portions: one for timing and the other one for charge measurements. Constant-fraction discriminators  $D_S$  (4F-163, Dubna designed) and  $D_M$  (Philips Scientific PS715) are attached to the

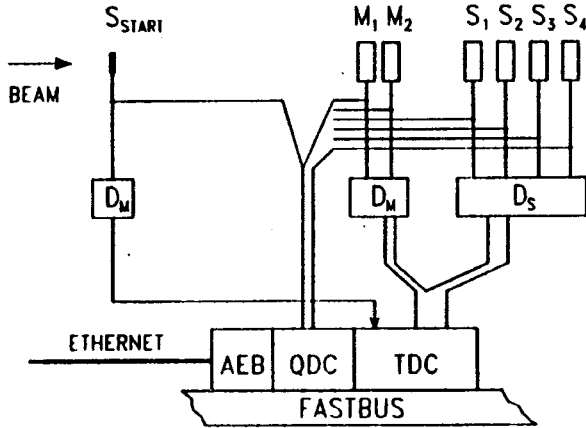


Fig.1. Schematic diagram of the measurements

counters  $S_1$ ,  $S_4$  and  $S_{Start}$ ,  $M_1$ ,  $M_2$ , respectively. Time between a signal of the start counter and signals of the counters under the test ( $\mathcal{T}_{Start-S_i}$ ,  $i = 1 \dots 4$ ) as well as integrated charge ( $Q_{S_i}$ ) of all signals were measured by FASTBUS TDC (Philips Scientific 10C6) and QDC (LeCroy 1882F). Data from TDC and QDC were read out by intelligent FASTBUS master AEB (Aleph Event Builder) and then transferred to SUN SPARCstation.

#### 4. Analysis and Results

Processing the data we eliminated a background by rejecting the events with the integrated charge being smaller than the lower bound for minimum ionizing particles (see Fig.2). When the elimination was applied, about 5 - 10% of the events were excluded from the data.

Some uncertainties in the beam contents and its momentum spread lead to the additional dispersion of the TOF value  $\mathcal{T}_{Start-S_i}$  measured at a long distance between the start counter and the counters under the test. By this reason as well as in order to exclude the influence of the start counter resolution we deal with the time differences for each two test counters:

$$\mathcal{T}_{S_i-S_j} = \mathcal{T}_{Start-S_i} - \mathcal{T}_{Start-S_j} \quad (1)$$

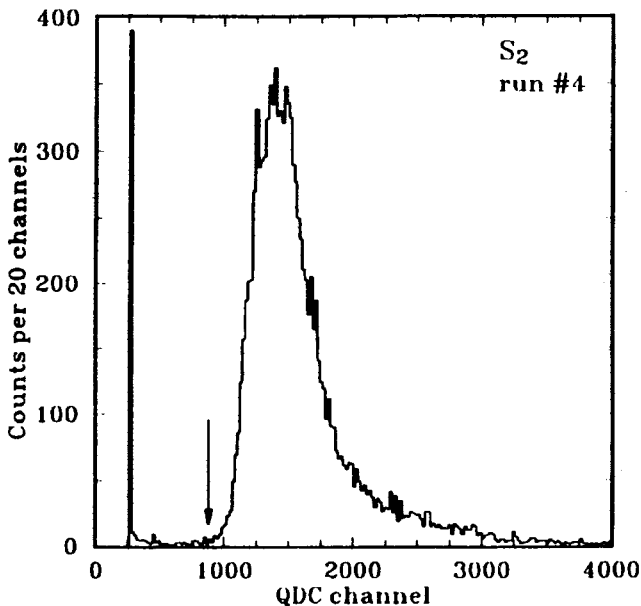


Fig.2. Integrated charge spectrum measured with  $S_2$  counter. The arrow shows the bound for elimination of background

Figure 3a shows typical scatter plot  $\mathcal{T}$  vs the integrated charge  $Q$  (the average value of  $\mathcal{T}$  is adjusted to be zero). We observed that the  $\mathcal{T}$  value depends on  $Q$  even for timing with the constant fraction method. This is the well-known time-walk effect and its magnitude is up to 200 ps in our case. As an attempt to correct the TOF measurements for this effect, fits to the data in the scatter plots were performed for each counter. The following function was used:

$$\mathcal{T}(Q_{S_i}) = P_{0i} + P_{1i}Q_{S_i} + P_{2i}Q_{S_i}^2 + P_{3i}Q_{S_i}^3 + P_{4i}Q_{S_i}^4 D, \quad (2)$$

where  $P_{0i}$ ,  $P_{4i}$  are the parameters for each counter.

Figure 3b shows a scatter plot between the corrected  $\mathcal{T}$  and  $Q$ . From this scatter plot we see that the time-walk effect has disappeared.

To obtain time resolutions  $\sigma_{S_i-S_j}$ , ( $i, j = 1 \dots 4, i \neq j$ ) the  $\mathcal{T}_{S_i-S_j}$  spectra were fitted with a Gaussian distribution (see for example Fig.4). Finally, we evaluated optimum values of the time resolutions  $\sigma_i$  for each individual counter using an asymptotic method. Table 1 shows the time resolutions for six runs distributed uniformly in time during 10-days test (about 60 runs). The errors presented are statistical ones.

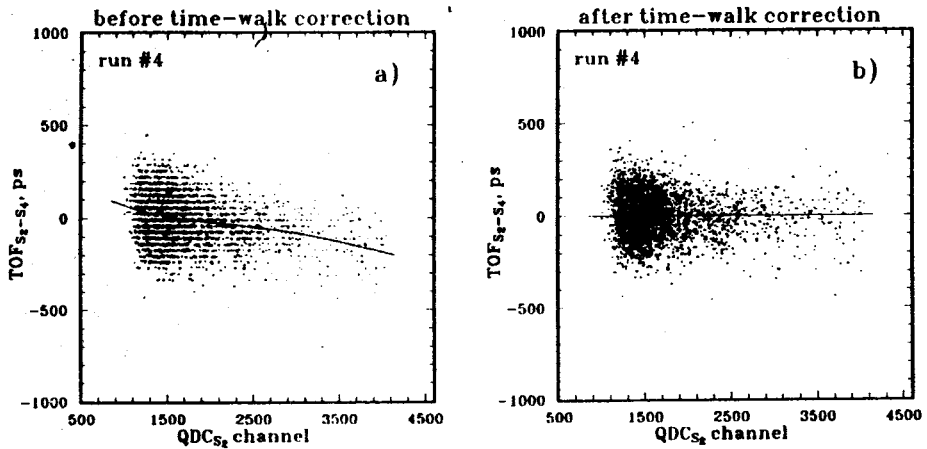


Fig.3. Scatter plot between the time-of-flight  $\mathcal{T}_{S_3-S_4}$  and the integrated charge  $Q_{S_2}$  before (a) and after (b) the time-walk correction

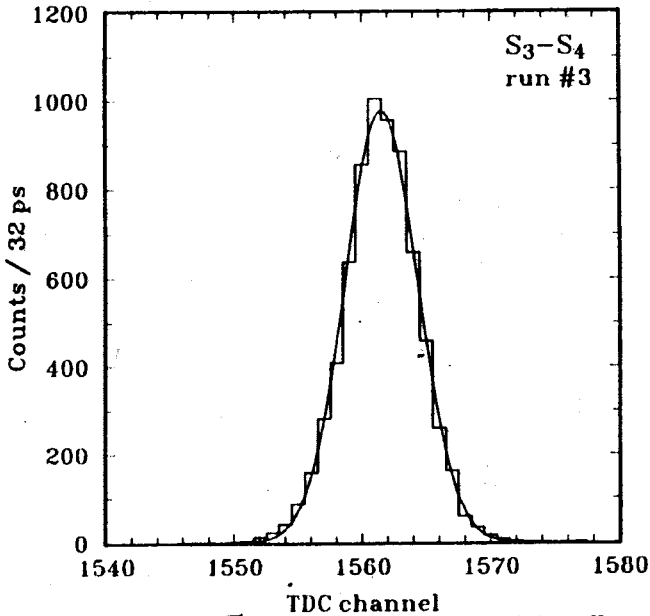


Fig.4. Time-of-flight  $\mathcal{T}_{S_3-S_4}$  spectrum after the time-walk correction. The solid curve is a Gaussian fit with  $\sigma = 91$  ps. Corresponding time resolutions of  $S_3$  and  $S_4$  counters are  $\sigma_3 = 74 \pm 9$  ps and  $\sigma_4 = 58 \pm 10$  ps

We note that the measured time resolutions are rather different for the same counters in various runs. One possible explanation of this fact could be connected with a conspicuous time drift of the counters. Fig-

**Table 1. The time resolution ( $\sigma$ ) of individual counters (CERN test)**

Run	# 1	# 2	# 3	# 4	# 5	# 6
Beam	20 GeV/c electrons	200 GeV/c protons				30 GeV/c protons
$\sigma_1$ , ps	$73 \pm 12$	$70 \pm 8$	$73 \pm 9$	$89 \pm 5$	$89 \pm 4$	$60 \pm 5$
$\sigma_2$ , ps	$72 \pm 13$	$82 \pm 7$	$82 \pm 10$	$79 \pm 5$	$78 \pm 5$	$80 \pm 3$
$\sigma_3$ , ps	$100 \pm 9$	$67 \pm 8$	$74 \pm 9$	$83 \pm 5$	$89 \pm 4$	
$\sigma_4$ , ps		$51 \pm 10$	$58 \pm 10$	$68 \pm 5$	$70 \pm 5$	$70 \pm 4$

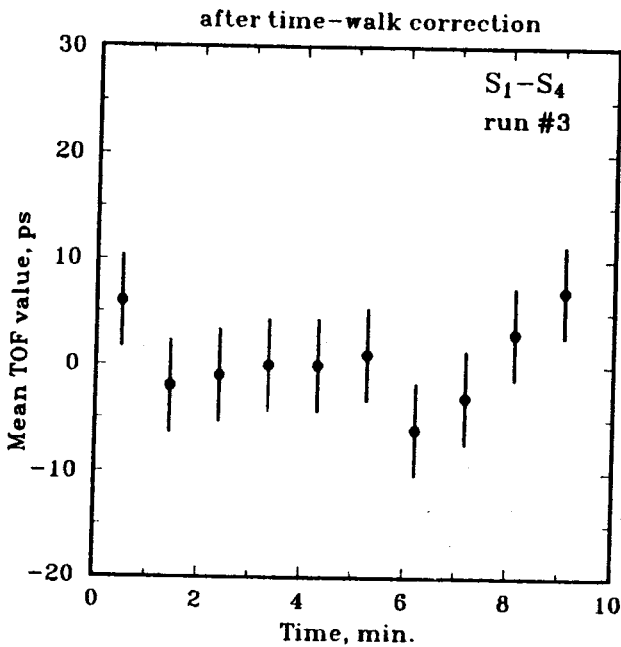


Fig.5. Typical drift of the mean  $\mathcal{T}_{S_1-S_4}$  value during the run.

Figure 5 shows a fluctuation of a mean value of  $\mathcal{T}_{S_1-S_4}$  between pulses from  $S_1$  and  $S_2$  counters during 10 minutes run #3. The typical time drift is estimated of 10–30 ps per run. However we observed a few runs with more unstable behaviour of some counters. For example, the time drift of  $\mathcal{T}_{S_2-S_3}$  (determined mainly by the contribution of the counter  $S_3$ ) in run #3 was about 80 ps. The time resolution  $\sigma_3$  extracted from initial 40% of the run events (with relatively low time drift) is equal to  $66 \pm 7$  ps ( $\sigma_3 = 74 \pm 9$  ps for whole run).

**Table 2. The time resolution ( $\sigma$ ) of individual counters (Dubna test)**

Run	# 1	# 2
Beam	6 GeV/c protons	
$\sigma_2$ , ps	$68 \pm 10$	$73 \pm 10$
$\sigma_3$ , ps	$57 \pm 12$	$61 \pm 12$
$\sigma_4$ , ps	$76 \pm 9$	$74 \pm 10$

Three months later we had a chance to repeat the TOF measurements with the same  $S_2$ ,  $S_3$ ,  $S_4$  counters at the JINR Synchrotron beam. The beam was 6 GeV/c protons. Each test run duration was approximately 4 hours. The detector time resolutions obtained by the described before procedure are presented in Table 2. We note that the time resolutions are similar to the measured before.

## 5. Conclusions

We tested the set of four scintillation TOF counters 6.0 cm long, 2.4 cm wide and 2.4 cm thick during a long-term run on the particle beam. The average time resolution ( $\sigma$ ) of about 70 ps is estimated for the whole test. This value includes the contribution of the TOF drift and, being corrected on the last one, the time resolution could be improved for up to (10–15)%.

The reproducibility of the timing results was tested and it appeared to be rather satisfactory.

Finally, in this work we have achieved the timing accuracy required by the planned experiment to have a good separation of pions, kaons and protons.

## 6. Acknowledgements

The work has been carried out owing to the support of the NA49 Collaboration members and we are very much obliged to them. Especially, we would like to express our gratitude to Prof. F.Puehlhofer, Drs. A.Piper and F.Eckhardt for this work could not have been done without their assistance.

We wish to thank Prof. A.M.Baldin for continuous support of our research program. The contribution of the SPHERE group (JINR) is acknowledged.

This work has been realized under promotion of the Russian Grant for Fundamental Research (93-02-3773).

## References

1. Large Acceptance Hadron Detector for an Investigation of Pb-Induced Reactions at CERN SPS. NA49 Collaboration, CERN SPSLC 91-31 SPSLC/P264.
2. Afanasiev S.V. et al. — JINR Rapid Communications, No.4[55]-92, Dubna, 1992, p.12.
3. Semenov A.Yu. et al. — Improved Scintillation Counters for Precise Time-of-Flight Measurements (to be published).
4. Matveeva E.N. et al.— Nucl. Instr. and Meth., 1981, 179, p.277.

Received on December 28, 1993.